

CHARACTERISTICS OF ELECTRODE MEMBRANE PVA-ENZIME COATING PVC-PLASTICIZER KTPCLPB FOR UREA BIOSENSOR

Evori N. Waruwu¹, Abd Hakim S.²
Physics Departement, Universitas Negeri Medan, Indonesia
e-mail: 1evorinatanaelwaruwu@gmail.com

ABSTRACT

This study aims to determine the effect of the composition comparison of the PVA-Enzyme urease coating PVC-Plastisizer KTpClPB membrane with memmbran characterization using FTIR and analyze membrane electrodes with XRD. The method used is the potentiometric method using the Electrode Selective Ion (ISE), where the polymer used is PVA and PVC as a coating with a composition ratio of PVA: PVC is 1: 1. The same PVA and PVC were used, namely 0.0350 g, with 2 mg of enzyme and 0.0500 g and 0.0120 g of KTpClPB plasticizer. The best composition result is the PVA-Enzyme PVC-Plastisizer coating enzyme KTpClPB 0.0500 g membrane electrode characterization using XRD shows the highest intensity value is at an angle of $2\theta = 44.020$ which is 1,626 count second (cts) and membrane characterization using FTIR shows that there is a functional group OH, CH, $C\equiv C$, NH, CO and CH. The addition of PVA-Enzyme coating will reduce or even eliminate the amount of Wolfram and can reduce the amorphous properties of the membrane electrodes.

Keywords: *Electrode Selective Ion (ISE), Potentiometric, PVA-Enzyme, PVC-Plastisizer KTpClPB*

INTRODUCTION

Biosensors are analytical tools that convert biological reactions into measurable signals such as electrical signals that allow it to analyze concentrations. The working principle of the biosensor is based on the immobilization of biological components (enzymes, bacteria, etc.) on the polymer membrane matrix which is integrated with the signal transducer on the analyte. The biological component functions as an electroactive sensor that plays a role in electrochemical half-cell reactions so that the potential generated is sensitive and selective to certain ions (Corcuera & Cavalieri, 2003).

The device developed based on the biological reaction (biocatalyst) "Urease" for analyzing urea is known as the urea biosensor. A urea biosensor is a device / biosensor that is made based on a signal from the urease "biocatalyst" reaction to urea to analyze urea levels in solution (Gupta, et al. 2010). The method of determining urea levels usually uses the spectrophotometric method, which is a method that uses the reaction between urea and diacetylmonoxime to produce a yellow color and the absorbance value is measured. The determination of urea by spectrophotometry is quite accurate, but it requires a relatively long time and a lot of chemicals. Therefore it is necessary to have a better method used in the determination of urea.

Another way to find out urea levels is by the potentiometric method. In the potentiometric method, the measurement of the equilibrium potential difference between the indicator electrode and the reference electrode will be measured

(Tamba, 2016). The indicator electrode is an electrode that is able to determine the change in concentration for a particular ion that corresponds to the enzyme on the electrode. One type of indicator electrode is the membrane indicator electrode, which is commonly called the Ion Selective Electrode (ISE), which is a membrane that allows certain types of ions to pass through but repels other types of ions (Arora, 2013). The problem that often occurs in the potentiometric method is the manufacture of membrane components to become biosensor samples. The electrode membrane (ISE) is the place where the potential or current is generated from the enzyme-catalyzed reaction on the electrode membrane with the solution being analyzed, so the electrode membrane parameters are very important because it will determine the biosensor's performance (Goncalves, 2014).

The electrode membrane parameters are determined by the type of supporting material or matrix chosen (Fauziyah, 2012). Therefore, various studies have been carried out using various types of polymers as urease immobilization matrix for membrane electrodes. One of them is the use of PVA polymer. PVA (Polyvinyl alcohol) is a water-soluble polymer that has great promise for biomedical applications. PVA is now known as a synthetic polymer which has been used as an interesting research material for immobilization of the "biocatalyst" in the form of a membrane. It is non-toxic and biocompatible with good chemical and thermal stability. The large number of hydroxyl groups in PVA provides a biocompatible microenvironment for the presence of enzymes (eg urease enzymes) (Kale, et al, 2016).

However, PVA is water soluble, so a waterproof but well-pore coating membrane is needed as a coating membrane. Research conducted by Tamba (2016) used PVA as the urease immobilization matrix. PVA was used as much as 0.5044 grams dissolved in water and mixed with 6 mg of urease. The coating membrane used was a 0.5044 gram PVC solution with 0.0120 KTpCIPB plasticizer and dissolved in THF. However, in his research, the correlation coefficient was 0.896. For this reason, changes will be made to the composition of the electrode membrane material, both in the composition of the PVA-enzyme membrane and the composition of the PVC-plasticizer membrane.

PVC is water-resistant and has good pores so it is suitable for use as a membrane. The use of plasticizers is needed to add elastic properties to PVC. Comparison of the composition of the PVC membrane and the plasticizer will affect the sensitivity and selectivity of the ISE membrane because the PVC membrane will coat the PVA membrane. The electrode membrane characterization was performed using X-ray diffraction (XRD) and the membrane characterization was performed using Fourier transform infrared spectroscopy (FTIR). FTIR is used to identify functional groups contained in a compound, and XRD is used to see the ratio of membrane intensity and characterize the resulting membrane (Hakim S, et al. 2018).

METHODS

The equipment used is XRD-6100 (Shimadzu), FTIR (Shimadzu), tungsten indicator electrode (W) and other supporting tools. The materials used in this study were 0.0350 g polyvinylalcohol (PVA), 2 mg of Urease enzyme (1%), 0.0350 g of polyvinylchloride (PVC), Pottasium tetrakis p-clorophenyl barate (KTpCIPb)

0.0120 g and 0,0500 g, Wolframm electrode with a diameter of 1 mm and a length of 4 cm, and the method used is the potentiometric method.

Comparison of the composition of the membrane used (W PVA: W PVC-plasticizer = 1: 1) where the mass of PVA and PVC are the same and the ratio of PVC: Plasticizer = 1: 2 (Hakim S, et al, 2018). In this study, researchers used PVC: KTpCIPB plasticizer with a ratio of 1:2. The preparation of the PVA-Enzyme solution comes from a mixture of the PVA solution and the enzyme solution. 0.0350 g PVA is dissolved in 10 mL of hot water to cold water, after which 2 mg of urease enzyme is dissolved in 0.5 mL consisting of water and alcohol with a ratio of 50% water: 50% alcohol. While the 0.0120 g KTpCIPB PVC-Plasticizer solution comes from mixing 0.0350 g PVC and 0.0120 g KTpCIPB dissolved into 10 mL THF in a beaker glass, and 0.0500 g KTpCIPB PVC-Plasticizer solution from mixing 0.0350 g PVC and 0.0500 g KTpCIPB which were dissolved in 10 mL THF in a beaker. So the PVA Enzyme solution and the PVC-Plasticizer KTpCIPB solution are used to form membranes and membrane electrodes. The membrane was characterized using FTIR, while the membrane electrode was characterized by XRD.

RESULT & DISCUSSION

Characterization of Membrane Electrodes Using XRD

The membrane electrode is made using a tungsten electrode rod with a different PVA-Enzyme coating. Sample I, sample II, sample III, respectively, are one layer, two layer membrane and three layers of PVA-Enzyme coated with composition I (PVC-Plasticizer KTpCIPB 0.0500 g). Sample IV, sample V and sample VI, respectively, are one layer, two layer membrane and three layers of PVA-Enzyme coated with composition II (PVC-Plasticizer KTpCIPB 0.0120 g). The characterization of membrane electrodes using XRD was carried out to determine the spectrum of wavelengths and the highest intensity values as well as the effect of adding a PVA-Enzyme layer from each sample of membrane electrodes in each composition.

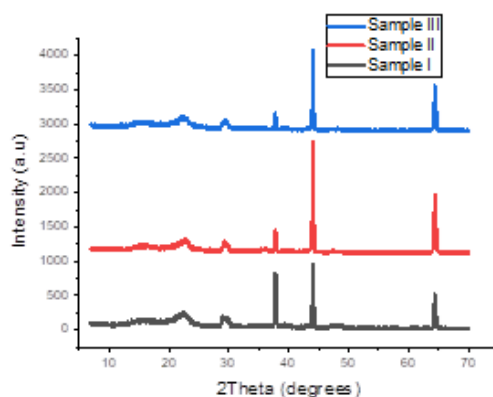


Figure 3.1 Diffraction pattern Samples of one, two and three layers of PVA-Enzyme coating composition I (PVC-Plasticizer KTpCIPB 0.0500 g)

In the diffraction pattern of Figure 3.1, there are five dominant diffraction peaks in each sample. In sample I (1 PVA-Enzyme layer) has diffraction peaks at $2\theta = 22.560; 28.940; 37.800; 44.020$ and 64.340 with the highest intensity value at the angle of $2\theta = 44.020$, namely 1,262 count second (cts). Sample II (2 PVA-Enzyme layers) had

diffraction peaks at $2\theta = 22.660$; 29.280 ; 37.780 ; 44.020 and 64.380 with the highest intensity value found at the angle of $2\theta = 44.020$, namely 1,626 count second (cts). And sample III (3 layers of PVA-Enzyme) has diffraction peaks at $2\theta = 22.220$; 29.560 ; 37.780 ; 44.020 and 64.380 with the highest intensity value at the angle of $2\theta = 44.020$, namely 1,174 count second (cts).

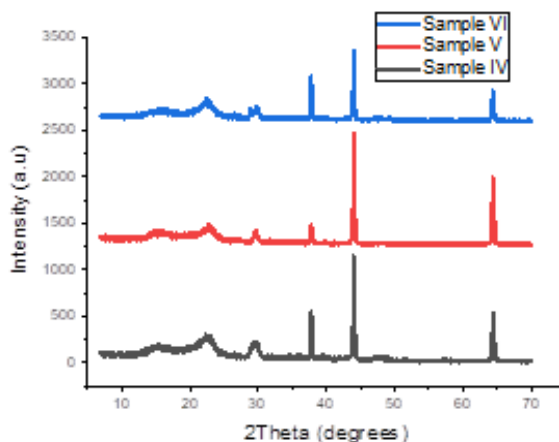


Figure 3.2 Diffraction pattern Samples of one, two and three layers of PVA-Enzyme coating composition II (PVC-Plasticizer KTpCIPB 0.0120 g)

In the diffraction pattern of Figure 3.2, there are five dominant diffraction peaks in each sample. In sample IV (1 PVA-Enzyme layer) has diffraction peaks at $2\theta = 22.400$; 29.420 ; 37.800 ; 44.040 and 64.400 with the highest intensity value found at the angle of $2\theta = 44.040$ which is 1,104 count second (cts). Sample V (2 PVA-Enzyme layers) had diffraction peaks at $2\theta = 22.600$; 29.640 ; 37.780 ; 44.000 and 64.380 with the highest intensity values found at the angle of $2\theta = 44,000$, namely 1,208 count second (cts). And sample VI (3 layers of PVA-Enzyme) has diffraction peaks at $2\theta = 22.520$; 29.660 ; 37.760 ; 44.000 and 64.320 with the highest intensity value at the angle of $2\theta = 44.020$, namely 770 count second (cts).

In general, polymer materials are semicrystalline, which means they have an amorphous and a crystalline part (Rohaeti, 2009). The diffraction pattern has peaks that are not sharp indicating a structure where this diffraction pattern is generally owned by semicrystalline materials (Yulianti, et al, 2013). In Figure 3.1 (PVA-Enzyme coating composition I), the diffraction pattern of the three samples has sharp peaks indicating crystalline properties and has non-sharp peaks indicating amorphous properties so it can be said that the sample is a semicrystalline material. Figure 3.2 (PVA-Enzyme coating composition II) also shows crystalline and amorphous properties so that the three samples are also semicrystalline materials.

In the diffraction pattern of sample I in Figure 3.1, it can be seen that the amorphous pattern at the beginning is higher than sample II and sample III. And so also in the diffraction pattern of sample IV in Figure 3.2 which shows a higher initial amorphous pattern than sample V and sample VI. This shows that the addition of a PVA-Enzyme layer in each composition reduces the amorphous properties of the membrane electrodes.

A good diffraction pattern can be seen from the intensity value obtained. The greater the intensity value obtained, the better the sample will be used (Hakim S, et al, 2019). The analysis above shows that the diffraction pattern that has the highest intensity value is sample II where the highest intensity value is 1,626 count second (cts) for the PVA-Enzyme coating membrane electrode composition I (PVC-Plasticizer KTpCIPB 0.0500 g) and sample V where the intensity value The highest was 1,208 count second (cts) for the electrode of the PVA-Enzyme coating composition II (PVC-Plasticizer KTpCIPB 0.0120 g).

Table 3.1 Compounds and Elements on PVA Membrane Electrodes-Enzyme coating composition I (PVC-Plasticizer KTpCIPB 0.0500 g)

Membrane Electrodes	Formula	Total (%)	Crystal System	Element
Sample I (1 PVA-Enzyme layer)	$C_6Cl_8N_{10}O_8$	44.6	Monoclinic	C, Cl, N, O
	$B_{10}ClH_{13}$	36.1	Monoclinic	B, Cl, H
	KNO_3	16.6	Orthorhombic	K, N, O
	$H_2O_7W_2$	1.8	Cubic	H, O, W
	Cl_5P	0.9	Tetragonal	Cl, P
Sample II (2 PVA-Enzyme layer)	$C_6Cl_8N_{10}O_8$	40.4	Monoclinic	C, Cl, N, O
	$Cl_{10}N_5P_5$	31.1	Orthorhombic	Cl, N, P
	$B_{10}Cl_2H_8P_2$	14.4	Orthorhombic	B, Cl, H, P
	KNO_3	13.6	Orthorhombic	K, N, O
	O_3W	0.5	Triclinic (anorthic)	Cl, K, O
Sample III (3 PVA-Enzyme layer)	$C_6Cl_8N_{10}O_8$	38.1	Monoclinic	C, Cl, N, O
	$B_{10}ClH_{13}$	37.8	Monoclinic	B, Cl, H
	KNO_3	22.8	Orthorhombic	K, N, O
	Cl_5P	1.3	Tetragonal	Cl, P

The components that are expected to be seen on the PVA-Enzyme PVC-Plasticizer coating enzyme KTpCIPB electrode are C, O, H, Cl, B, P, K, and W (Hakim S, et al, 2017). In table 3.1, samples I and II of the PVA-Enzyme coating coating electrode compoai I (PVC-Plasticizer KTpCIPB 0.0500 g) have complete elements, namely elements C, O, H, Cl, B, P, N, K, and W Likewise with samples IV and V of the PVA-Enzyme coating coating electrode composition II (PVC-Plasticizer KTpCIPB 0.0120 g) has complete elements, namely elements C, O, H, Cl, B, P, N, K, and W shown in table 3.2. This shows that the membrane electrode is formed from the PVA-Enzyme membrane, PVC-Plasticizer KTpCIPB and tungsten rods.

Based on the characterization carried out for the membrane electrode with three layers of PVA-Enzyme (sample III and sample VI), no W element was seen. This indicated that the membrane was made too thick so that the tungsten rod was covered by the membrane. The addition of the PVA-Enzyme layer on the tungsten rod can affect the amount of W element present in the membrane electrodes.

Table 3.2 Compounds and Elements on the PVA Membrane Electro-Enzyme coating composition II (PVC-Plastisizer KTpCIPB 0.0120 g)

Membrane Electrodes	Formula	Total (%)	Crystal System	Element
Sample IV (1 PVA-Enzyme layer)	C ₁₂ N ₁₈ O ₈	77.6	orthorhombic	C, N, O
	BH ₉ N ₃ P	9.6	Monoclinic	B, H, N, P
	P	8.4	Triclinic (anorthic)	P
	N ₄ W ₃	2.5	Cubic	N, W
	ClKO ₄	1.9	orthorhombic	Cl, K, O
Sample V (2 PVA-Enzyme layer)	C ₁₂ N ₁₈ O ₈	80.6	orthorhombic	C, N, O
	K ₄ O ₇ P ₂	9.7	Hexagonal	K, O, P
	BH ₉ N ₃ P	4.8	Monoclinic	B, H, N, P
	ClKO ₄	2.6	orthorhombic	Cl, K, O
	O ₇ P ₂ W	2.2	Cubic	O, P, W
Sample VI (3 PVA-Enzyme layer)	C ₁₂ N ₁₈ O ₈	70.9	orthorhombic	C, N, O
	O ₇ P ₄	17.5	Monoclinic	O, P
	BHO ₂	11.1	Cubic	B, H, O
	ClKO ₄	0.5	orthorhombic	Cl, K, O

Membrane Characterization Using FTIR

Based on the results of the analysis using XRD, a good sample is sample II (2 layers of PVA-Enzyme PVC-Plastisizer coating 0.0500 g KTpCIPB) for composition I and sample V (2 layers of PVA-Enzyme PVC-Plastisizer coating 0.0120 g KTpCIPB) for composition II. The membrane that has been made based on a good sample of each composition will be characterized using FTIR to determine the functional groups contained in the membrane. Figure 3.3 below shows the FTIR spectrum graph of the PVA-Enzyme PVC-Plastisizer KTpCIPB membrane (0.0500 g and 0.0120 g).

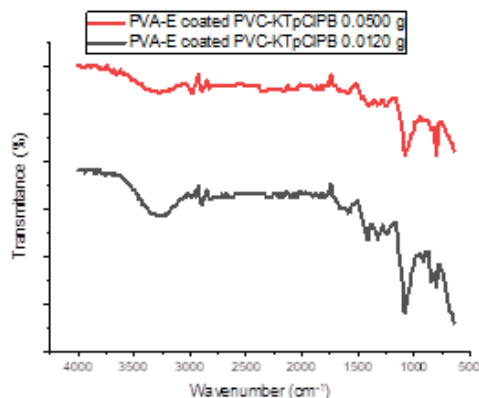


Figure 3.3 FTIR spectrum on a 2 layer PVA membrane-enzyme coating PVC-Plastisizer KTpCIPB (0.0500 g and 0.0120 g)

Based on Figure 3.3, on the PVA-E 2X membrane 0.0500 g KTpCIPB PVC-P and 2X PVA-E membrane. PVC-P KTpCIPB 0.0120 g contained the CH functional group seen in the wave numbers 2,850-2,970 cm^{-1} , 1,340-1,470 cm^{-1} , and 3,010-3,100 cm^{-1} groups. The OH functional group is seen in the wave number group 3,200-3,650 cm^{-1} and the NH functional group is seen in the 3200-2400 cm^{-1} group. Groups of wave numbers at 1,000-1,250 cm^{-1} and 1,500-1,750 cm^{-1} indicate the presence of a CO functional group. It can be seen that there is a $\text{C}\equiv\text{C}$ functional group in the wave number group 2,100-2,300 cm^{-1} , but not very prominent.

At 1,000-1,250 cm^{-1} and 1,340-1,470 cm^{-1} wavelengths, the CH and CO functional groups were seen on the PVA-E 2X membrane. 0.0500 g KTpCIPB PVC-P stands out more than the PVA-E 2X membrane. PVC-P KTpCIPB 0.0120 g. Then the OH functional group was also more prominent on the PVA-E 2X membrane. PVC-P KTpCIPB 0.0500 g. This shows that the addition of the PVC-Plasticizer KTpCBIB composition will increase the number of transmittances (%) on several functional groups found on the PVA-Enzyme PVC-Plasticizer KTpCIPB membrane.

CONCLUSION

Based on the results of the analysis of membrane electrode characterization using XRD, it is known that the best intensity is found in the PVA-Enzyme coated with composition I (PVC-Plasticizer KTpCIPB 0.0500 g) with the highest intensity value at the angle of $2\theta = 44.020$, namely 1,626 count second (cts). And based on the analysis of membrane characterization on composition I and II using FTIR, the functional groups of CH, OH, NH, CO, and $\text{C}\equiv\text{C}$ were obtained. It was concluded that the addition of the PVA-Enzyme layer would reduce the amorphous properties of the membrane electrodes, and the addition of the PVC-Plasticizer KTpCBIB composition would increase the number of transmittances (%) in several functional groups found on the membrane.

BIBLIOGRAPHY

- Arora, N. (2013). Recent Advances in Biosensors Technology: A Review. *Octa Journal of Biosciences*, 1 (2) : 147-150.
- Corcuera, D. R. J., & Cavalieri, P. R. (2003). Biosensor. *Encyclopedia of Agricultural, Food, and Biological Engineering*.
- Fauziyah, B. (2012). Optimasi Parameter Analitik Biosensor Urea Berbasis Immobilisasi Urease dalam Membran Polianilin. *Saintis*, 1 (1) : 65-72.
- Goncalves, A. M., Pedro, A. Q., Santos, F. M., Martins, L. M., Maia, C. J., Queiroz, J. A., & Passarinha, L. A. (2014). Trends in Protein-Based Biosensor Assemblies for Drug Screening and Pharmaceutical Kinetic Studies. *Molecules*, www.mdpi.com/journal/19.
- Gupta, B., Singh, S., Mohan, S., & Prakash R. (2010). Urea Biosensor based on Conducting Polymer Transducers. *Biosensor*. India, Intech.55
- Hakim S, A., Tarigan, K., Sebayang, K., Sembiring, T., & Sitomurang, M. (2017). The Characteristic Membrane PVA-Enzim and Coating PVC-Plasticizer with XRD. *The 4th Annual International Seminar on Trends in Science and Science Education State University of Medan* 32-40



- Hakim S, A., Tarigan, K., Sebayang, K., Sembiring, T., & Sitomurang, M. (2018). The Characteristic Mebrane PVA-Enzim and Coating PVC-Plastisizer with SEM-EDX. *International Journal of Scientific & Engineering Research*, **9**(1) : 1229-1236.
- Hakim S, A., Tarigan, K., Sitomurang, M., & Sembiring, T. (2018). Synthesis of Urea Sensors using Potentiometric Methods with Modification of Electrode Membranes Indicators of ISE from PVA-Enzymes Coating PVC-KTpClPB. *The 8th International Conference on Theoretical Applied Physics*, 1-14.
- Hakim S, A., Sembiring, T., Tarigan, K., Sebayang, K., Situmorang, M., & Noer, N. M. (2019). Characterization of Membrane PVA-Enzyme Coating PVC-KTpClPB as Urea Sensor with Potentiometric Method. *RASAYAN J. Chem*, **12** (2) : 780-786.
- Kale, P. D., Bodade, A. B., & Chaudhari, G. N. (2016). Study of Immobilization of Urease on PVA-Nano NiFe₂O₄ Nanocomposite for Biosensor Application. *International Journal of Pharmacy and Pharmaceutical Science*, **8** (7) : 380-385.
- Rohaeti, E. (2009). Karakterisasi Biodegradasi Polimer. *Prosiding Seminar Nasional Penelitian dan Penerapan MIPA, UNY*, 248-257.
- Tamba, D. (2016). Immobilisasi Enzim Urease untuk Pembuatan Sensor Kimia dalam Penentuan Urea. Skripsi, FMIPA, UNIMED, Medan.
- Yulianti, E, Saputri R. D., Sudaryanto, Jodi, H., & Salam, R. (2013). Pembuatan Bahan polimer Elektrolit Padat Berbasis Nanokomposit Kitosan Montmorillonite untuk Aplikasi Baterai, *Jurnal Kimia Kemasan* **35** (2) ; 77-83